


Dr. Name _____ Phone # _____
 Acct. # _____ Patient Name _____
First Last
 Address/Email _____ **Deliver by 5 p.m. on** _____
 Enclosed with Case: Impressions Models Bite Photos Other: _____

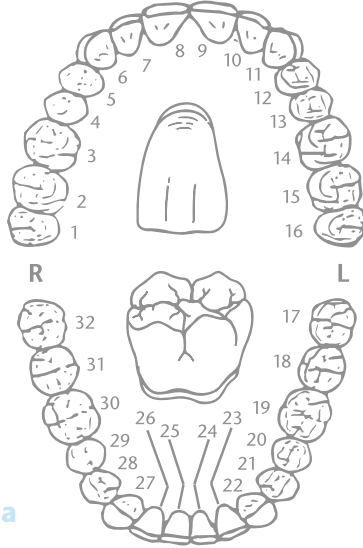

All Restorations
Made in California

Signature _____
 License # _____
(see reverse for limited warranty details)

SCREW-RETAINED RESTORATIONS <input type="checkbox"/> Obsidian Fused to White Noble Metal <input type="checkbox"/> Obsidian Fused to White High Noble <input type="checkbox"/> Captek YHN <input type="checkbox"/> BruxZir Full-Strength* (1,150 MPa) (w/ Ti-Base) <input type="checkbox"/> NEW! BruxZir Esthetic (870 MPa) (w/ Ti-Base) <input type="checkbox"/> IPS e.max (w/ Ti-Base)	SELECT ABUTMENT TYPE Inclusive Custom Implant Abutments <input type="checkbox"/> Titanium Abutment* <input type="checkbox"/> Zirconia w/ Ti-Base <input type="checkbox"/> Prepare existing abutment <input type="checkbox"/> White noble abutment See reverse for implant systems supported
PORCELAIN FUSED TO METAL <input type="checkbox"/> Obsidian Fused to Non-Precious* <input type="checkbox"/> Obsidian Fused to White Noble <input type="checkbox"/> Obsidian Fused to White High Noble <input type="checkbox"/> Captex YHN <input type="checkbox"/> OcclusalGold YHN	ALL-CERAMICS & ZIRCONIA <input type="checkbox"/> BruxZir Full-Strength* (1,150 MPa) <input type="checkbox"/> NEW! BruxZir Esthetic (870 MPa) (stump shade recommended for restorations less than 1.5 mm thick) <input type="checkbox"/> PrismaTik CZ <input type="checkbox"/> Lava <input type="checkbox"/> IPS e.max
COMPOSITE RESTORATIONS <input type="checkbox"/> Lava Ultimate <input type="checkbox"/> Camouflage Composite <input type="checkbox"/> with fiber reinforcement	


VIVANEER VENEER
 Conventional-Prep:
 BruxZir Esthetic IPS e.max
 Minimal-Prep:
 IPS e.max

FULL-CAST RESTORATIONS
 Noble-Cast 45 YN* (40% Au) Non-precious
 Noble-Cast 60 YHN (52% Au) Semi-precious
 Noble-Cast 67 YHN (64% Au) WHN (40% Au)
 OcclusalGold YHN (73.1% Au) Post & core
 JRVY YHN (77% Au)

NIGHTGUARDS/BITE SPLINTS/ MOUTHGUARDS
 Upper Lower
 Comfort H/S Bite Splint* (hard/soft)
 Soft nightguard Comfort Bite Splint (hard)
 PlaySafe Mouthguards
 Jr Lt Lt Pro Med Hvy Hvy Pro
 Helmet strap (available in red or black)
 Name _____ (specify colors on Rx)


PROVISIONALS
 Transition C&B
 Abutment #(s) _____
 Pontic #(s) _____ Total units _____
 Splinted units* Individual units
 BioTemps Provisionals
 Reinforcement: None Wire* Fiber
 BioTemps with Cast-Metal Substructure
 Amount of prep reduction:
 1 mm* 2 mm
 Perio treatment: Prepare tooth below gingival on tooth #(s) _____ by _____ mm
 Pontic site healing: Prepare ovate socket on tooth #(s) _____ by _____ mm



***Standard unless otherwise specified**

FINAL SHADE
 _____

STUMP SHADE
Must indicate prepped tooth shade for all-ceramics

OCCUSAL STAINING
 None Light* Medium Dark

PONTIC DESIGN


MARGIN AND METAL DESIGN

 Labial Butt Junction * Junct. Collar

 Excl. Cusp Incl. Cusp

DENTURES/FLIPPERS/FLEXIBLE PARTIALS
 Simply Natural Digital Dentures
 Valplast tcs DuraFlex
 saddles/clasps
 Vitallium 2000 Vitallium 2000 Plus
 Kenson Teeth (Included at no extra charge)
 Premium Brand Teeth (Extra charge applies)
 Shade _____ Mould _____

IF NO OCCUSAL CLEARANCE
 Call doctor Spot opposing Metal occlusion
 Would you like this to be a permanent note?
 Yes No

NOTE: Metal linguals at lab's discretion

IN-LAB WORKING TIMES

Please allow full working time for each product selected. Working times are NOT guaranteed and do NOT include weekends or holidays. Rush service available but must be prescheduled.

IN-LAB WORKING TIMES

Obsidian Fused to Metal	5 days
Obsidian w/ attachment or implant	7 days
Full-cast restorations	4 days
All-ceramic/BruxZir Solid Zirconia	5 days
Composite	6 days
Prismatik Clinical Zirconia	8 days
Custom Implant Abutments	8 days
Lava	11 days
BioTemps Provisionals	5 days
with cast-metal substructure	6 days


Transition Crowns & Bridges	5 days
Nightguards/Bite splints	5 days
Custom tray	3 days
Bleaching tray	5 days
PlaySafe sports mouthguards	4 days

All rush cases must be prescheduled by calling our Customer Service department before the case is shipped. Time of pickup and delivery may affect turnaround time.

To schedule your rush case, call 800-321-9943.


PREPARATION GUIDELINES

OBSIDIAN TO METAL ANTERIOR




- A. 2 mm incisal reduction
- B. 1.5 mm middle third reduction
- C. Labial and lingual walls must be convergent
- D. Preparation should be cut in three planes

OBSIDIAN TO METAL POSTERIOR

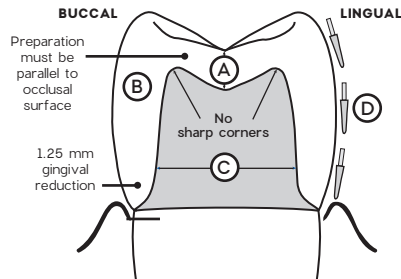


- A. 2 mm occlusal reduction
- B. 1.5 mm middle third reduction
- C. Buccal and lingual walls must be convergent
- D. Preparation should be cut in three planes

OBSIDIAN TO METAL – CERAMIC LABIAL OR 360° MARGIN

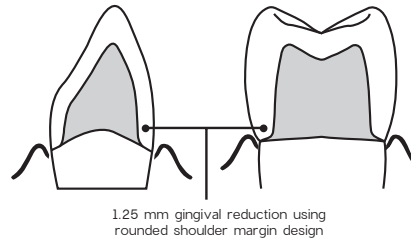


1.25 mm gingival reduction using rounded shoulder margin design

ALL-CERAMIC/COMPOSITE VENEERS

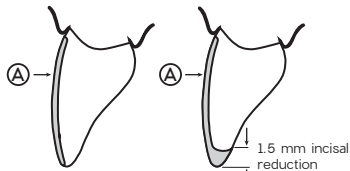


- A. 0.3 to 1 mm labial reduction

INLAY




- A. 1.5 to 2 mm occlusal reduction
- B. Round all sharp line angles and occlusal edges, and eliminate undercuts
- C. Proximal and occlusal walls should have 6–8 degrees taper

ONLAY



ALL-CERAMIC/COMPOSITE CROWNS

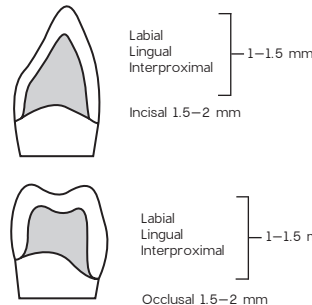

TERMS AND WARRANTY INFORMATION

We honor VISA, MASTERCARD, AMEX and DISCOVER.

TERMS: Cost of collection of any account will be paid by the customer. All accounts are payable within 30 days of statement date. *Accounts not paid within the stated terms will be subject to COD status and a late charge of 2 percent of the unpaid balance.* Prices subject to change without notice. Rx must be enclosed with original case submission.

LIMITED WARRANTY/LIMITATION OF LIABILITY. Riverside Dental Ceramics ("the lab") warrants that all dental devices (a "device") are made according to your specification and approval in the belief that the device will be useful and MAKES NO OTHER WARRANTIES INCLUDING, BUT NOT LIMITED TO, ANY IMPLIED WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. Subject to the return of a device that is placed and then fails, the lab will repair or replace the device without charge for the cost of materials and workmanship or refund the original price paid, at the lab's option, as follows: (1) screw-retained implant abutments up to 20 years (including replacement of a device that was made by the lab that was attached to said abutments and including an Inclusive® Tapered titanium dental implant upon request at no extra charge); (2) porcelain to metal, all ceramic, all metal, single-unit inlay, onlay and crown composite resin final prosthetics, and screw-retained crowns and implant bars, up to seven years; (3) composite resin bridges (excluding Maryland and inlay/onlay bridges) up to five years; (4) Transition Crowns and Bridges® up to two years; (5) thermoformed appliances and splints if the failure is due to defects in materials or workmanship, provisionals, composite resin Maryland and inlay/onlay bridges, up to six months; (6) all other dental devices up to 30 days if the failure is due to defects in materials or workmanship. This Warranty is exclusively for your benefit, is not transferable and does not extend to any patients. You agree to pay all other costs of adjustment, repair and replacement of a device. Except where prohibited by law, the lab WILL NOT BE LIABLE FOR ANY LOSS OR DAMAGES ARISING FROM THE USE OF A DEVICE, WHETHER DIRECT, INDIRECT, SPECIAL, INCIDENTAL OR CONSEQUENTIAL, regardless of the theory asserted, including warranty, contract, negligence or strict liability and if such disclaimer is not permitted by law, the duration of any implied warranty is limited to 90 days from the date of delivery. In the event of a dispute and absent an amicable resolution the parties mutually agree to waive class actions in favor of mandatory individual arbitration of claims under this limited warranty in and in accordance with the laws of California. The lab does not guarantee the performance of independent carriers.